


AERODYNE RESEARCH, Inc.

Aerosol Mass Spectrometer

Description

The Aerodyne AMS provides quantitative real-time, size-resolved composition analysis of non-refractory particulate matter. Aerosol particles in the size range 0.04 to ~1.0 micrometers are sampled into a high vacuum system where they are aerodynamically focused into a narrow beam (~1 mm diameter). The particle beam is directed onto a resistively heated surface where volatile and semivolatile chemical components are thermally vaporized and detected via standard 70 eV electron impact ionization quadrupole mass spectrometry. Particle aerodynamic diameter is determined from particle time-of-flight (velocity) measurements using a beam chopping technique.

This approach provides universal detection of chemical species that vaporize (in <1 sec) at 200 to 900 C (typically 600 C). This non-refractory fraction includes the majority of atmospheric components, with the notable exception of elemental carbon and crustal oxides (dust). Some inorganic components (e.g., sea-salt) require vaporization at higher temperature (900 C).

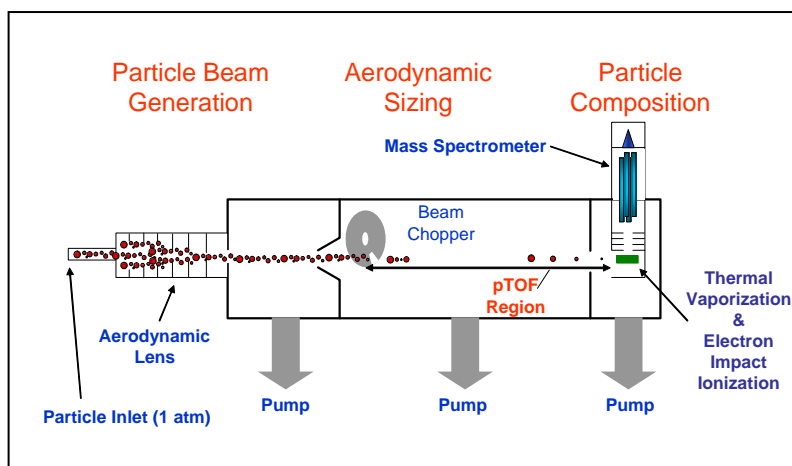

The combination of quantitative size and chemical analysis of sub-micron aerosol mass loadings with fast time resolution makes the Aerodyne AMS unique. Other aerosol instrumentation can provide complementary information. For example, differential mobility analyzers count and size ultrafine particles (no chemical analysis), which often have too little mass for effective AMS detection. Laser based time-of-flight particle mass spectrometer systems obtain mass spectra of individual (> 0.2 μm) particles, enabling separation of internal vs. external chemical mixing, but lack quantitative analysis due to non-linearities in the laser-ablation/ionization process.

The latest version of the AMS utilizes a time-of-flight mass spectrometer (ToF-AMS) which increases sensitivity, while enabling complete single particle analysis. The high resolution HR-ToF-AMS has high mass resolving power (up to 4000), enabling elemental analysis (C, H, O, N) for $m/z < 100$ and the potential to resolve other chemical components such as metals (e.g., Fe, Zn, Pb, Hg) and PAHs. Other options include an optical light scattering module that enables simultaneous optical, aerodynamic and chemical particle analysis (for $d > 200$ nm).

The AMS has been successfully deployed on mobile platforms (including sampling exhaust plumes from on-street vehicles), research vessels, and aircraft. The Aerodyne AMS is the only currently available instrument capable of providing quantitative size and chemical mass loading information in real-time for non-refractory sub-micron aerosols.

For more information see the two websites below

http://www.aerodyne.com/products/aerosol_mass_spectrometer.htm

<http://cires.colorado.edu/~jjose/ams.html>

ARI Aerosol Mass Spectrometer Models

Quadrupole-AMS



Compact-ToF-AMS



High Resolution-ToF-AMS



Three versions of the AMS are available: Quadrupole-AMS (Q-AMS), Compact-ToF-AMS (C-ToF-AMS) and High Resolution-ToF-AMS (HR-ToF-AMS). Attributes are summarized below:

	<u>Detection Limit*</u> ($\mu\text{g}/\text{m}^3$)	<u>Mass Resolving Power</u> (m/ Δ m)	<u>Mass Range</u> (m/z)
Q-AMS	0.01	300	1-300
C-ToF-AMS	0.002	800	1-1000
HR-ToF-AMS (V-mode)	0.003	2000	1-1200
HR-ToF-AMS (W-mode)	0.05	4000	1-1200

* Detection limits depend on chemical species. Typical values for nitrate are listed.

Call to discuss custom applications and components under development, such as, alternate soft ionization schemes, particle lenses for larger and smaller sizes, and light scattering modules:

Dr. Douglas R. Worsnop
 Vice President
 Director, [Center for Aerosol and Cloud Chemistry](#)
 Phone: 978-663-9500, ext. 225
 Fax: 978-663-4918
 e-mail: worsnop@aerodyne.com

Mrs. Cameron Martin
 Executive Assistant, Marketing Director
[Center for Aerosol and Cloud Chemistry](#)
 Phone: 978-663-9500, ext. 207
 Fax: 978-663-4918
 e-mail: cmartin@aerodyne.com

Dr. John Jayne
 Co-Director, [Center for Aerosol and Cloud Chemistry](#)
 Phone: 978-663-9500, ext. 233
 Fax: 978-663-4918
 e-mail: jayne@aerodyne.com

AERODYNE RESEARCH, Inc.

AMS Instrument Specifications

April, 2008

Performance

- Size resolved mass analysis of non-refractory aerosol components.
- Chemical analysis by thermal vaporization and electron impact ionization mass spectrometry
- Q-MS: unit mass resolution to 300 amu, scan rate 1 msec/amu.
- ToF-MS – mass range up to m/z 1200, mass resolving power ($m/\Delta m$) up to 4000.
- Real-time mass spectral analysis of inorganic (nitrate, sulfate, ammonium) and organic mass (OM).
- Particle vaporization temperature adjustable from 200 C to 900 C
- Single particle detection diameter approximately 200 nm.
- Sensitivity of ~ 0.002 to $0.05 \mu\text{g}/\text{m}^3$ in a minute – depends on chemical species and MS option.
- Sampling flow rate 85 cc min^{-1} .
- Aerodynamic particle size measurement in the range of 40 nm to $\sim 1 \mu\text{m}$. Size resolution of 5 to 10 ($D_{\text{aero}}/\Delta D_{\text{aero}}$, FWHM) over that size range.
- Fast time resolution of seconds. Maximum data rate $\sim 100 \text{ Hz}$.
- Data output format; ASCII, HDF. Wavemetrics© Igor program license supplied.
- Acquisition and analysis software included (free upgrades).

Physical

<u>Size</u>	Approximately 41"W x 24"D x 53"H.
<u>Weight</u>	Approximately 170 kg.
<u>Power</u>	Approximately 600 Watts. Universal power 110VAC/60Hz or 220VAC/50Hz. Vacuum system fully operational on 24 VDC.
<u>Computer</u>	Current systems are shipped with rack a mounted computer, PIII 3GHz, Intel Core™ 2 Duo Processor, 512M SDRAM, 160G hard drive, CD-RW, floppy, 10/100 Ethernet port, 8 USB ports, 1 serial port. Flat screen monitor 17" XGA.
<u>Packaging</u>	Shipped in one reusable container. Total shipping weight $\sim 280 \text{ kg}$. Approx. outside dimensions of container 30"W x 51"L x 63"H on fork lift skids, for Q-AMS, and 30"W x 51"L x 58" H for C- and HR-ToF-AMS.

AMS OPTIONS

Light Scattering Module provides additional information for larger particles (>200nm), particularly for large refractory (dust) particles with low non-refractory coatings. Light scattering analysis also can provide information on particle density and distinguish internal/external mixtures.

Negative Ion Detection Option for ToF-AMS (via electron attachment) selectively detects stable anion species, such as sulfate, nitrate and carboxylic acids. Sensitivity is 1000 lower than electron impact (EI). Switchable with standard EI.

Relative Humidity/Temperature/Pressure probes allow the user to measure ambient relative humidity, temperature and pressure at sampling inlet, with all measurements fully integrated into the data acquisition system.

Beam Width Probe allows measurement of particle shape by measuring the divergence of the particle beam.

Service/Support Contract (3 years) includes spare parts (extra filaments and electron multiplier) and up to two weeks of on-site support. Parts and support are interchangeable, as needed, based on advance payment of fee. Parts will usually be shipped overnight.

AMS COMPONENTS UNDER DEVELOPMENT

Soft Ionization Schemes provide less molecular fragmentation than electron impact ionization. Li⁺ ion attachment, VUV photo-ionization, and low energy electron attachment with negative ion mode detection are under development.

Black Carbon Detection Module relies on laser-induced incandescence vaporization for black carbon containing aerosol particles. This allows simultaneous quantification of the organic, inorganic and black carbon components of aerosol particles.

Aerodynamic Lens development is ongoing. A PM_{2.5} lens with a transmission range from 200 nm to 2.5 μm has been tested, as has a nanolens with transmission from 30 nm to 300 nm

LIST OF SELECTED AMS PUBLICATIONS

A complete list of publications related to the AMS and electronic files are available at <http://cires.colorado.edu/jimenez/ams-papers.html>.

Jayne, J.T., D.C. Leard, X. Zhang, P. Davidovits, K.A. Smith, C.E. Kolb, and D.R. Worsnop, Development of an aerosol mass spectrometer for size and composition analysis of submicron particles, *Aerosol Sci. Technol.*, 33, 49-70, 2000.

Jimenez, J.L., J.T. Jayne, Q. Shi, C.E. Kolb, D.R. Worsnop, I. Yourshaw, J.H. Seinfeld, R.C. Flagan, X. Zhang, K.A. Smith, J. Morris, and P. Davidovits, Ambient Aerosol Sampling with an Aerosol Mass Spectrometer. *J. Geophys. Res. - Atmospheres*, 108(D7), 8425, doi:10.1029/2001JD001213, 2003.

Zhang, X., Smith, K.A., Worsnop, D.R., Jimenez, J.L., Jayne, J.T., and Kolb, C.E. A Numerical Characterization of Particle Beam Collimation by an Aerodynamic Lens-Nozzle System. Part I: An Individual Lens or Nozzle. *Aerosol Science and Technology*, 36: 617–631 (2002).

- Allan, J.D., Jimenez, J.L., Coe, H., Bower, K.N., Williams, P.I., and Worsnop, D.R. Quantitative Sampling Using an Aerodyne Aerosol Mass Spectrometer. Part 1: Techniques of Data Interpretation and Error Analysis. *Journal of Geophysical Research – Atmospheres*, Vol. 108, No. D3, 4090, doi:10.1029/2002JD002358, 2003.
- Allan, J.D., Coe, H., Bower, K.N., Williams, P.I., Gallagher, M.W., Alfarra, M.R., Jimenez, J.L., Worsnop, D.R., Jayne, J.T., Canagaratna, M.R., Nemitz, E., and McDonald, A.G. Quantitative Sampling Using an Aerodyne Aerosol Mass Spectrometer. Part 2: Measurements of Fine Particulate Chemical Composition in Two UK Cities. *Journal of Geophysical Research – Atmospheres*, Vol. 108, No. D3, 4091, doi:10.1029/2002JD002359, 2003.
- Drewnick, Frank, James J. Schwab, John T. Jayne, Manjula Canagaratna, Douglas R. Worsnop, Kenneth L. Demerjian. Measurement of Ambient Aerosol Composition during the PMTACS-NY 2001 using an Aerosol Mass Spectrometer. Part I: Mass Concentrations. *Aerosol Science & Technology*, 38(S1):92–103, 2004.
- Drewnick, Frank, James J. Schwab, John T. Jayne, Manjula Canagaratna, Douglas R. Worsnop, Kenneth L. Demerjian. Measurement of Ambient Aerosol Composition during the PMTACS-NY 2001 using an Aerosol Mass Spectrometer. Part II: Chemically Speciated Mass Distributions. *Aerosol Science & Technology* 38(S1):104–117, 2004.
- Bahreini, R., J.L. Jimenez, J.T. Jayne, D.R. Worsnop, R.C. Flagan, and J.H. Seinfeld, Aircraft-based Aerosol Mass Spectrometer Measurements of Particle Size and Composition during ACE-Asia, *Journal of Geophysical Research – Atmospheres* 108, 8645, doi:10.1029/2002JD003226, 2003.
- Canagaratna, Manjula R., John T. Jayne, David A. Ghertner, Scott Herndon, Quan Shi, Jose L. Jimenez, Philip J. Silva, Paul Williams, Thomas Lanni, Frank Drewnick, Kenneth L. Demerjian, Charles E. Kolb, Douglas R. Worsnop, Chase Studies of Particulate Emissions from in-use New York City Vehicles, *Aerosol Science & Technology* 38:555–573, 2004.
- Schneider, J., S. Borrmann, A. G. Wollny, M Bläsner, N Mihalopoulos, K Oiconomou, J Sciare, ATeller, Z Levin, D R. Worsnop, On-line mass spectrometric aerosol measurements during the MINOS campaign (Crete, August 2001), *Atmos. Chemistry and Physics (ACP)*, 4, 65-80, 2004.
- Zhang, Q., C.O. Stanier, M.C. Canagaratna, J.T. Jayne, D.R. Worsnop, S.N. Pandis, and J.L. Jiménez, Insights into the Chemistry of Nucleation Bursts and New Particle Growth Events in Pittsburgh Based on Aerosol Mass Spectrometry, *Env. Sci. and Tech.*, 38, 4797-4809, 2004.
- Schneider, J., N. Hock, S. Weimer, S. Borrmann, U. Kirchner, R. Vogt, V. Scheer, Nucleation particles in diesel exhaust: Composition inferred from in-situ mass spectrometric analysis, *Environmental Science and Technology*, 39,6153-6161, 2005.
- Takegawa, N., Y. Kondo, Y. Komazaki, Y. Miyazaki, T. Miyakawa, J. L. Jimenez, J. T. Jayne, D. R. Worsnop, J. D. Allan, and R. J. Weber. Characterization of an Aerodyne Aerosol Mass Spectrometer (AMS): Long-Term Stability and Intercomparison with Other Aerosol Instruments. *Aerosol Science and Technology*, 39:760–770, 2005.
- Kolb, C. E.; Herndon, S. C.; McManus, J. B.; Shorter, J. H.; Zahniser, M. S.; Nelson, D. D.; Jayne, J. T.; Canagaratna, M. R.; Worsnop, D. R. Mobile Laboratory with Rapid Response Instruments for Real-Time Measurements of Urban and Regional Trace Gas and Particulate Distributions and Emission Source Characteristics. *Environ. Sci. Technol.* 38(21): 5694-5703, 2004.
- de Gouw, J.A., A.M. Middlebrook, C. Warneke, P.D. Goldan, W.C. Kuster, J.M. Roberts, F.C. Fehsenfeld, D.R. Worsnop, M.R. Canagaratna, A.A.P. Pszenny, W.C. Keene, M. Marchewka, S.B. Bertman, T.S. Bates. The Budget of Organic Carbon in a Polluted

- Atmosphere: Results from the New England Air Quality Study in 2002. *J. of Geophys. Res. – Atmos.*, 110, D16305, doi:10.1029/2004JD005623, 2005.
- Drewnick, F., S.S. Hings, P.F. DeCarlo, J.T. Jayne, M. Gonin, K. Fuhrer, S. Weimer, J.L. Jimenez, K.L. Demerjian, S. Borrmann, D.R. Worsnop. A new Time-of-Flight Aerosol Mass Spectrometer (ToF-AMS) – Instrument Description and First Field Deployment. *Aer. Sci. Technol.*, 39:637–658, 2005.
- Zhang, Q., Douglas R. Worsnop, Manjula R. Canagaratna, and Jose-Luis Jimenez. Hydrocarbon-like and Oxygenated Organic Aerosols in Pittsburgh: Insights into Sources and Processes of Organic Aerosols. *Atmospheric Chemistry and Physics*, 5, 3289-3311, 2005.
- Marr, L.C., K. Dzepina, J. L. Jimenez, F. Riesen, H. L. Bethel, J. Arey, J. S. Gaffney, N. A. Marley, L. T. Molina, M. J. Molina. Sources and transformations of particle-bound polycyclic aromatic hydrocarbons in Mexico City. *Atmos. Chem. and Physics Discuss.*, 5, 12741-12773, 2005.
- Zhang, Q., M. Rami Alfarra, Douglas R. Worsnop, James D. Allan, Hugh Coe, Manjula R. Canagaratna, and Jose L. Jimenez. Deconvolution and quantification of hydrocarbon-like and oxygenated organic aerosols based on aerosol mass spectrometry. *Environmental Science and Technology*, 39: 4938-4952, 2005, doi:10.1021/es048568l.
- DeCarlo, P.F., J.R. Kimmel, A. Trimborn, M.J. Northway, J.T. Jayne, A.C. Aiken, M. Gonin, K. Fuhrer, T. Horvath, K. Docherty, D.R. Worsnop, and J.L. Jiménez, A Field-Deployable High-Resolution Time-of-Flight Aerosol Mass Spectrometer, *Analytical Chemistry*, 78, 8281-8289, 2006.
- Canagaratna, M.R., J.T. Jayne, J.L. Jiménez, J.D. Allan, M.R. Alfarra, Q. Zhang, T.B. Onasch, F. Drewnick, H. Coe, A. Middlebrook, A. Delia, L.R. Williams, A.M. Trimborn, M.J. Northway, P.F. DeCarlo, C.E. Kolb, P. Davidovits, and D.R. Worsnop, Chemical and Microphysical Characterization of Ambient Aerosols with the Aerodyne Aerosol Mass Spectrometer, *Mass Spectrometry Reviews*, 26, 185-222, 2007.
- Cross, E.S., J.G. Slowik, P. Davidovits, J.D. Allan, D.R. Worsnop, J.T. Jayne, D.K. Lewis, M. Canagaratna, and T.B. Onasch, Laboratory and Ambient Particle Density Determinations using Light Scattering in Conjunction with Aerosol Mass Spectrometry, *Aerosol Sci. Tech.*, 41, 343-359, 2007.
- Northway, M.J., J.T. Jayne, D.W. Toohey, M.R. Canagaratna, A. Trimborn, K.-I. Akiyama, A. Shimono, J.L. Jiménez, P.F. DeCarlo, K.R. Wilson, and D.R. Worsnop, Demonstration of a VUV lamp photoionization source for improved organic speciation in an aerosol mass spectrometer, *Aerosol Science & Technology*, 41, 829-839, 2007.