




Dual Laser Trace Gas Monitor

Sensitive, rapid, highly specific and continuous measurements of multiple atmospheric trace gases in ambient air.

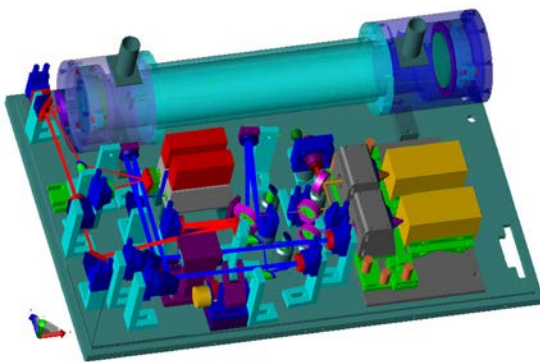

APPLICATIONS

- Extremely sensitive detection of a wide variety of atmospheric trace gases, such as: methane, nitrous oxide, nitric oxide, nitrogen dioxide, carbon monoxide, carbon dioxide, formaldehyde, formic acid, ethylene, acetylene, carbonyl sulfide, acrolein, ammonia and others.
- Combustion monitoring and characterization.
- Isotopic monitoring of CH_4 and N_2O for source/sink characterization.
- Eddy Covariance measurements.
- Fast response plume studies.
- Air quality monitoring.
- Mobile measurements from ship, truck, and Aircraft platforms.

ADVANTAGES

- Absolute trace gas concentrations with out calibration gases.
- Fast time response.
- Free from interferences by other atmospheric gases or water vapor.
- Turnkey and unattended operation.
- Ready to be deployed in field measurements and on moving platforms.
- Two lasers allow simultaneous measurement of more species.
- Optical pathlength of either 76 meters or 210 meters.



POPULAR INSTRUMENTS

HIGHER PRECISION AND ACCURACY IS OBTAINABLE WITH MID-INFRARED LASERS



Clumped CO₂ Isotopes*



CH₄ Isotopes



CO₂, Water Isotopes



N₂O Isotopes



NO, NO₂



CH₄, N₂O, CO, CO₂, H₂O

MECHANICAL SPECIFICATIONS FOR DUAL LASER TRACE GAS MONITOR:

Dimensions: 560 mm x 770 mm x 640 mm (W x D x H)

Weight: 75 kg

Electrical Power: 250-500 W, 120/240 V, 55/60 Hz (without pump)

MULTIPASS CELL:

Choice of 76 meter standard cell (V=0.5 liters) or 210 meter "Super Cell" (V=2liters)

*Image attribution by Psammophile [GFDL (<http://www.gnu.org/copyleft/fdl.html>) or CC-BY-SA-3.0-2.5-2.0-1.0 (<http://creativecommons.org/licenses/by-sa/3.0>)], via Wikimedia Commons

REFERENCES:

Nelson, D.D. et al., Optics Let. 31, 2012-2014, 2006.

McManus, J.B. et al., Applied Physics B, DOI: 10.1007/s00340-006-2407-7 (2006).

McManus, J.B., M.S. Zahniser, D.D. Nelson, L.R. Williams, and C.E. Kolb, Infrared laser spectrometer with balanced absorption for measurements of isotopic ratios of carbon gases., Spectrochim. Acta A, 58, 2465-2479, (2002).

McManus, J.B., D.D. Nelson, J.H. Shorter, R. Jiménez, S. Herndon, S. Saleska, and M.S. Zahniser, A high precision pulsed QCL spectrometer for measurements of stable isotopes of carbon dioxide, J. Modern Optics, 52, 2309-2321 (2005).

Saleska, SR; J. Shorter, S. Herndon, R. Jimenez, B. McManus, D. Nelson, M. Zahniser, What are the instrumentation requirements for measuring the isotopic composition of net ecosystem exchange of CO₂ using eddy covariance methods? Isotopes in Environmental and Health Studies, 42 (1), 117 (2006).

Nelson, D.D., J. B. McManus, S. C. Herndon, M. S. Zahniser, B. Tuzson and L. Emmenegger, New Method for Isotopic Ratio Measurements of Atmospheric Carbon Dioxide Using a 4.3 μm Pulsed Quantum Cascade Laser, Appl. Phys. B 90, 301-309 (2008).

Tuzson, B, J. Mohn, M. J. Zeeman, R. A. Werner, W. Eugster, M. S. Zahniser, D. D. Nelson, J. B. McManus, L. Emmenegger, High precision and continuous field measurements of δ¹³C and δ¹⁸O in carbon dioxide with a cryogen-free QCLAS, Appl. Phys. B 92, 451-458 (2008).